

FIG. 1B

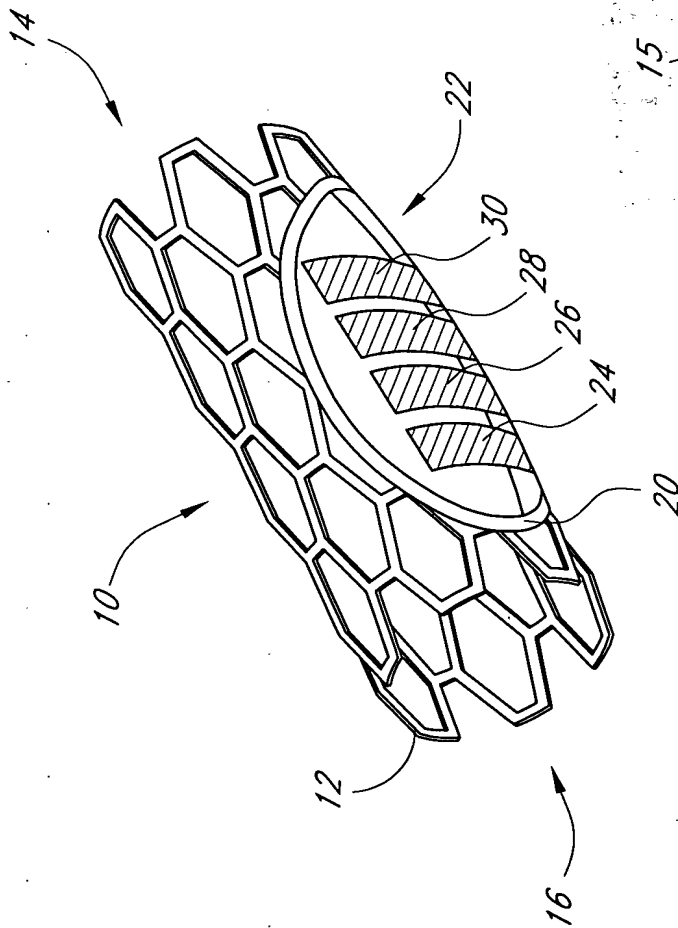


FIG. 1A

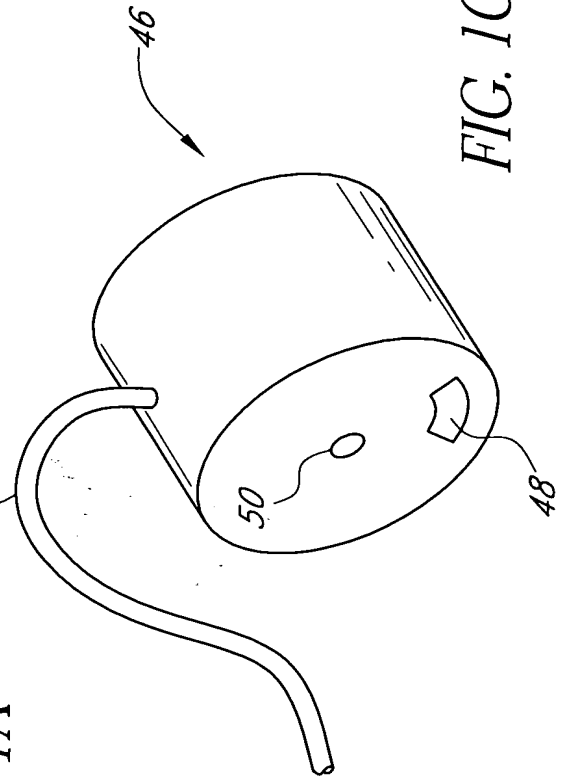


FIG. 1C

2/22

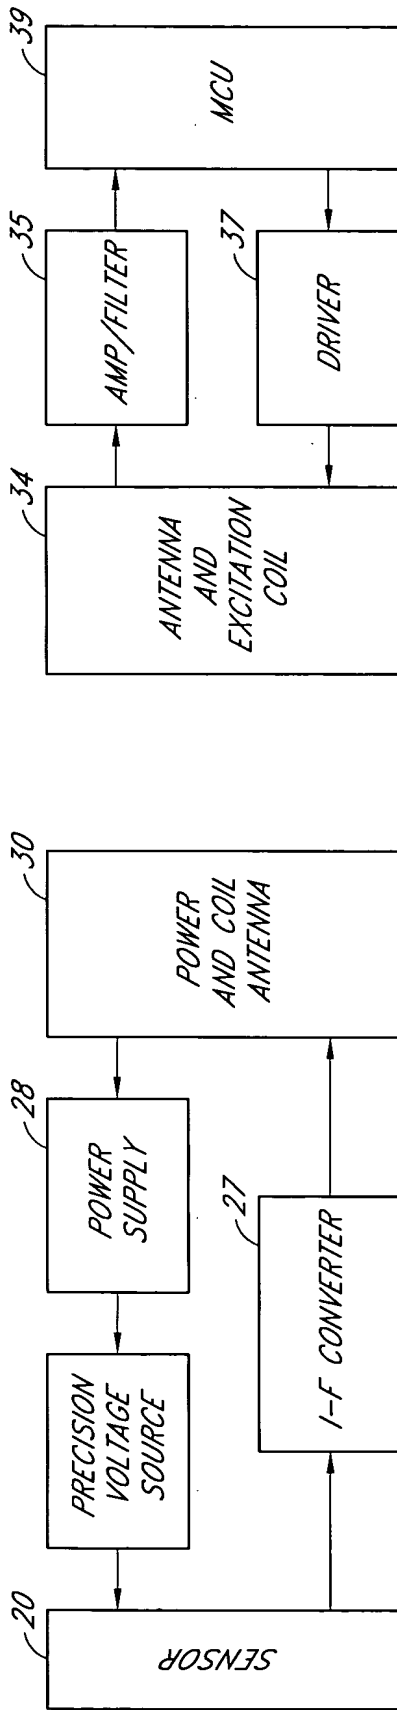


FIG. 1E

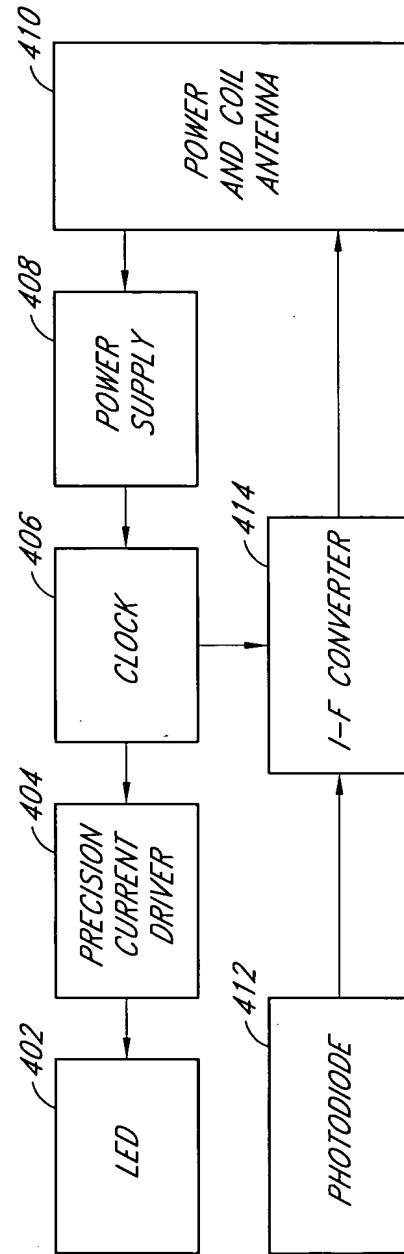


FIG. 13

IMPLANTABLE, RETRIEVABLE, THROMBUS MINIMIZING SENSORS

James H. Silver

Appl. No.: Unknown Atty Docket: JSILVER.1CP2CP

3/22

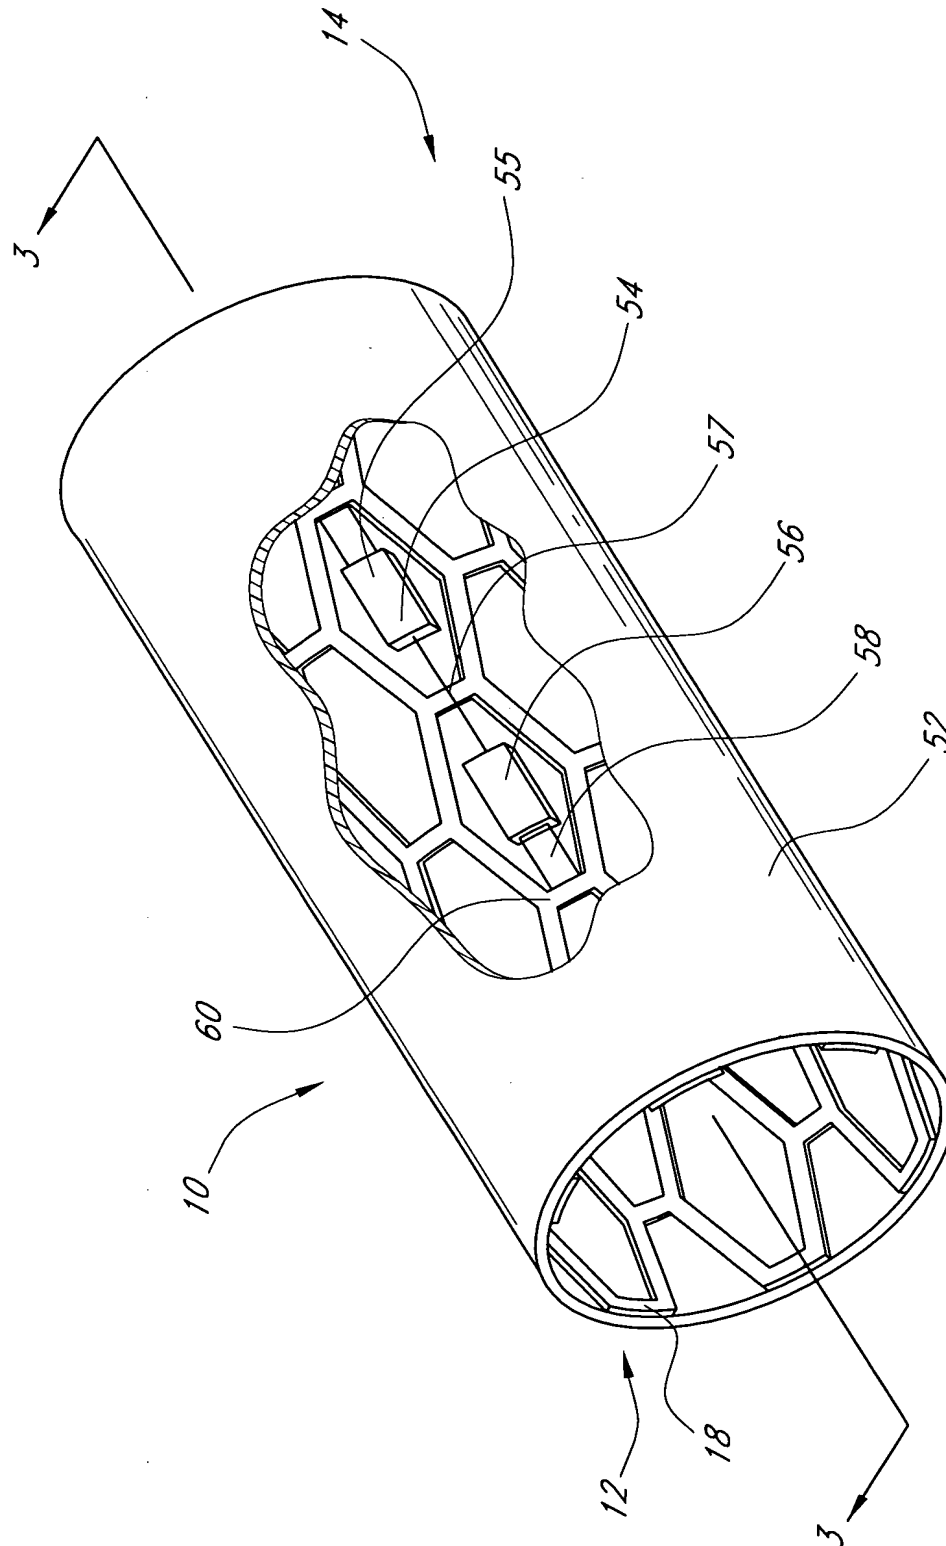


FIG. 2

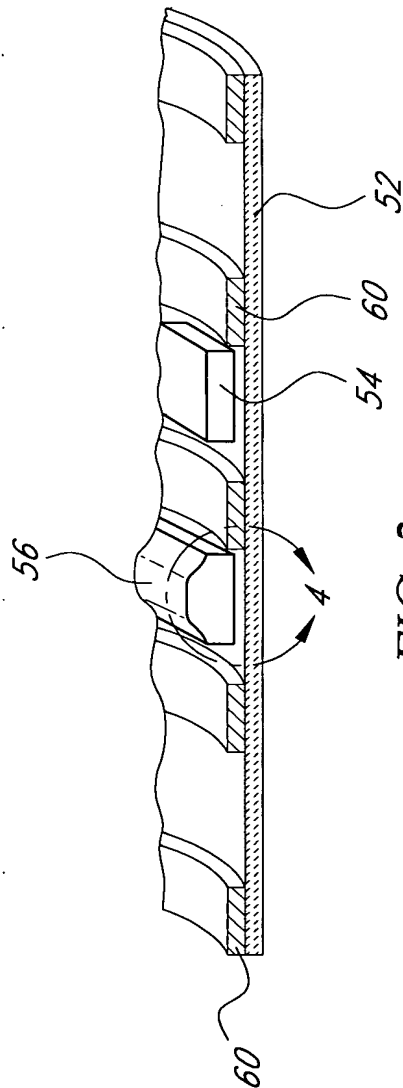


FIG. 3




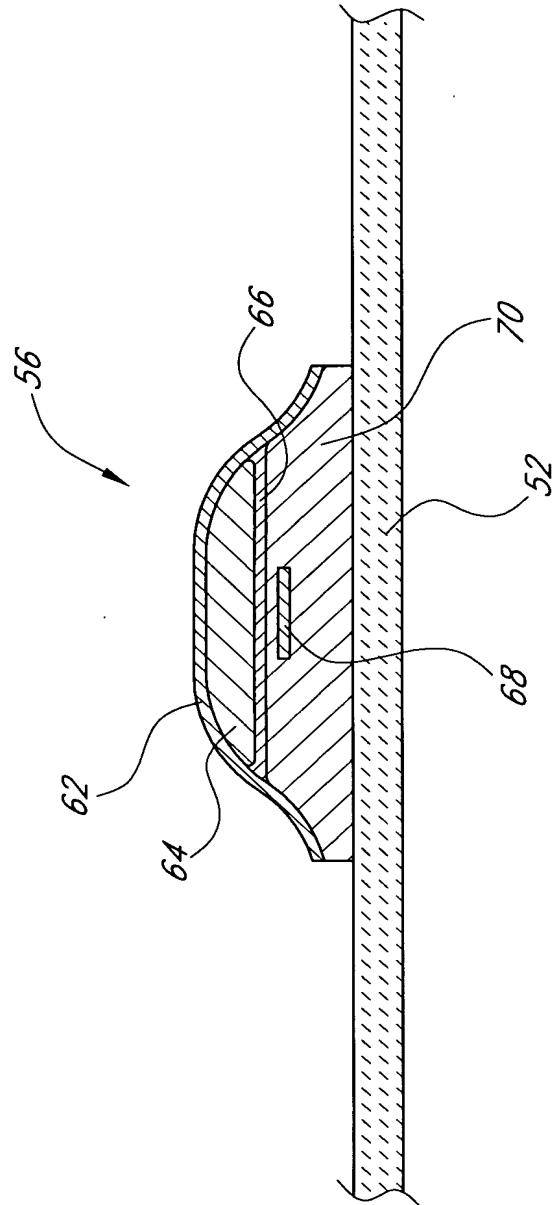


FIG. 4

IMPLANTABLE, RETRIEVABLE, THROMBUS MINIMIZING SENSORS

James H. Silver

Appl. No.: Unknown Atty Docket: JSILVER.1CP2CP

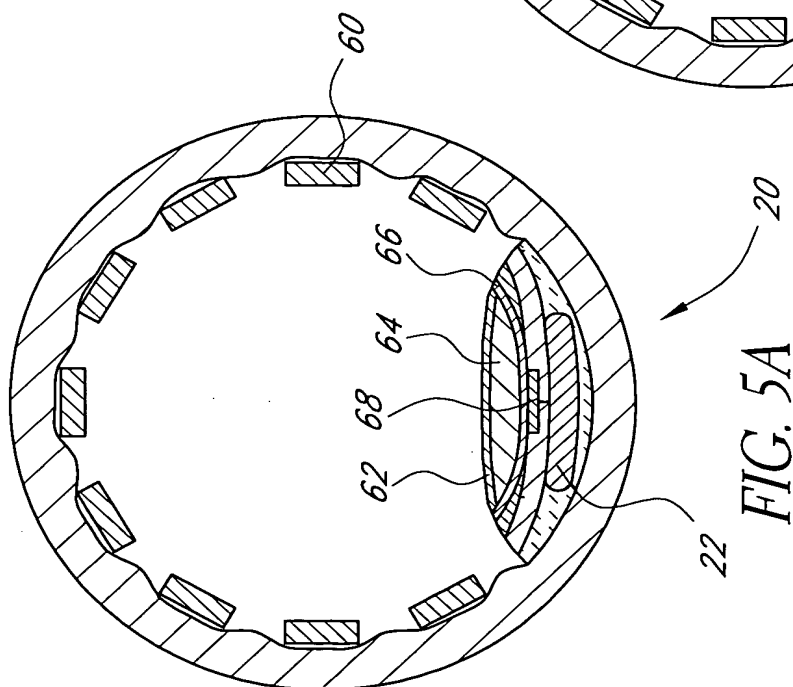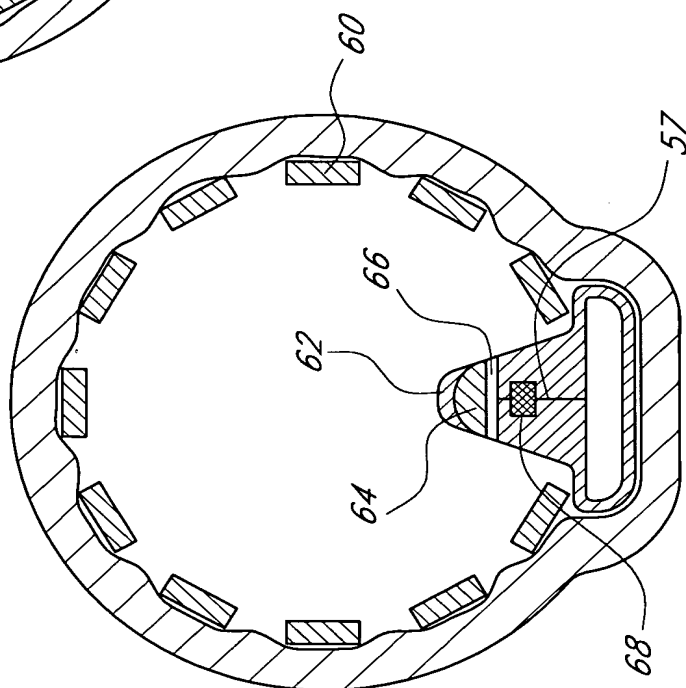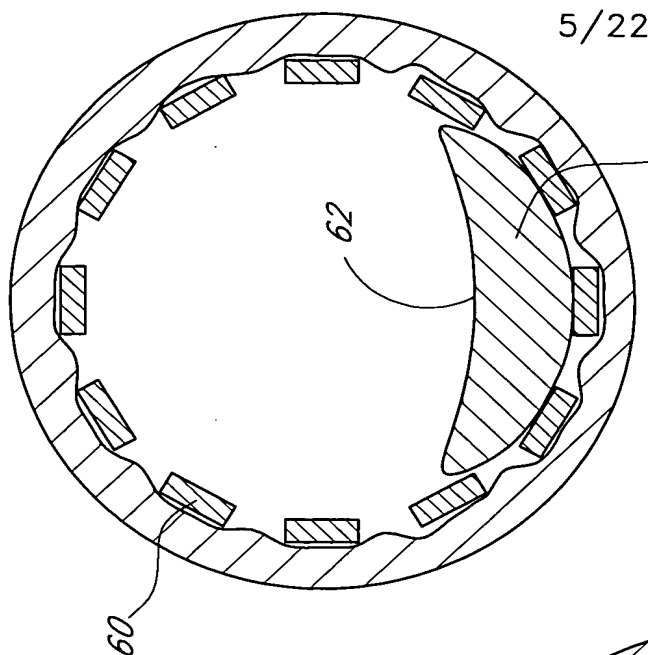

6/22

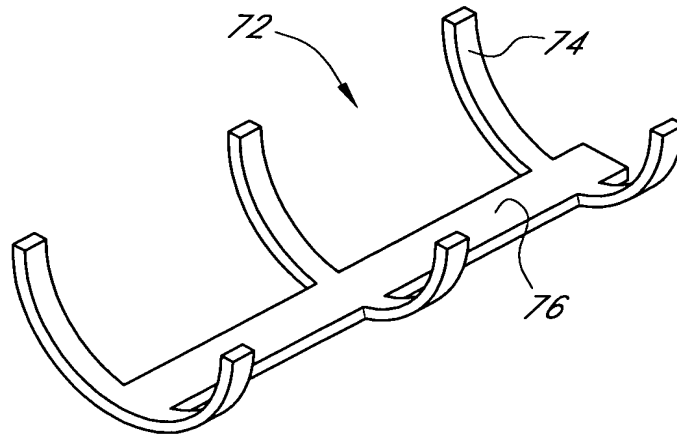


FIG. 6A

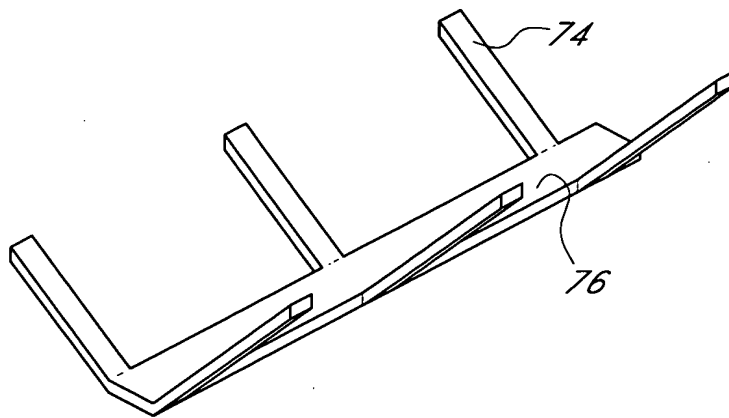


FIG. 6B






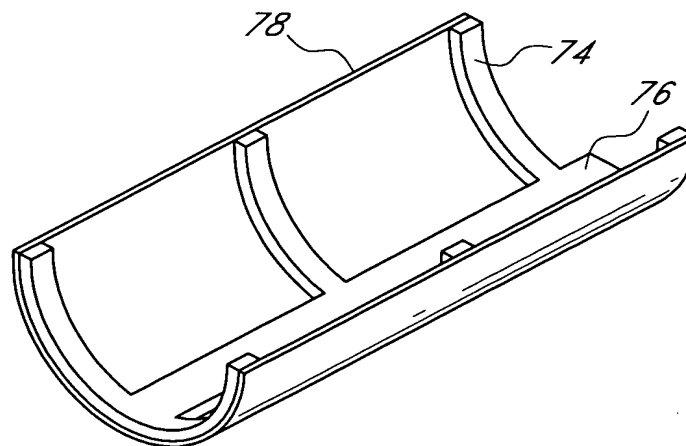


FIG. 6C


7/22

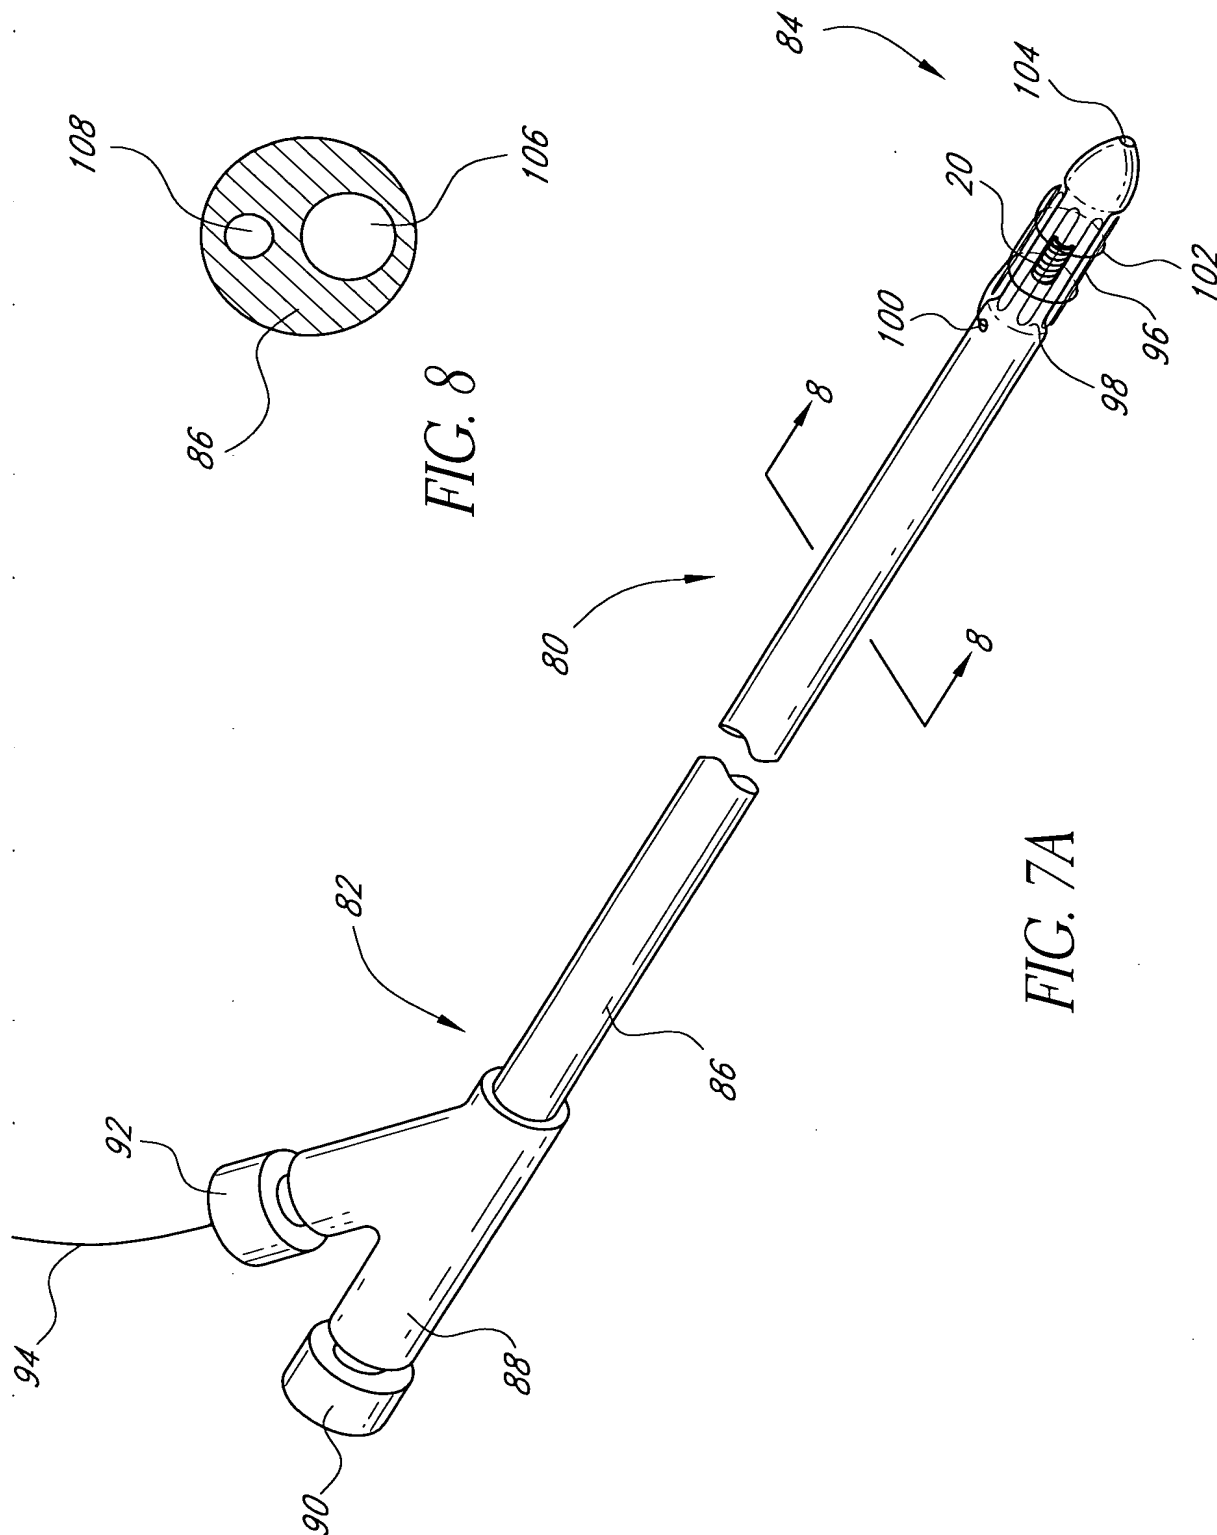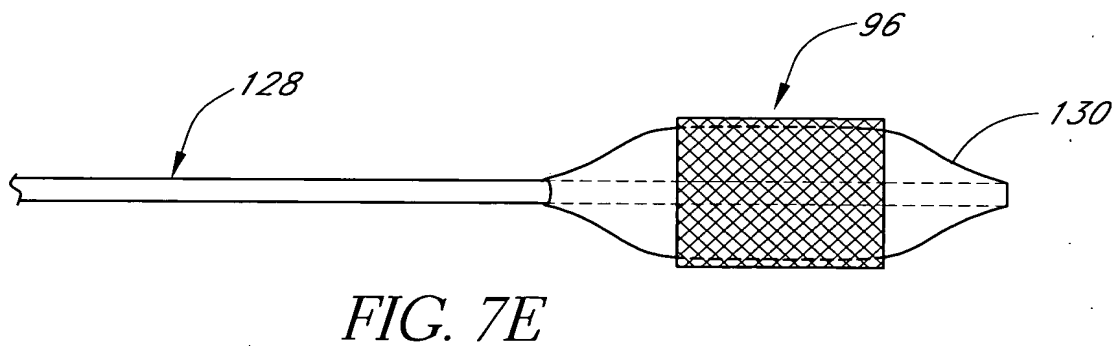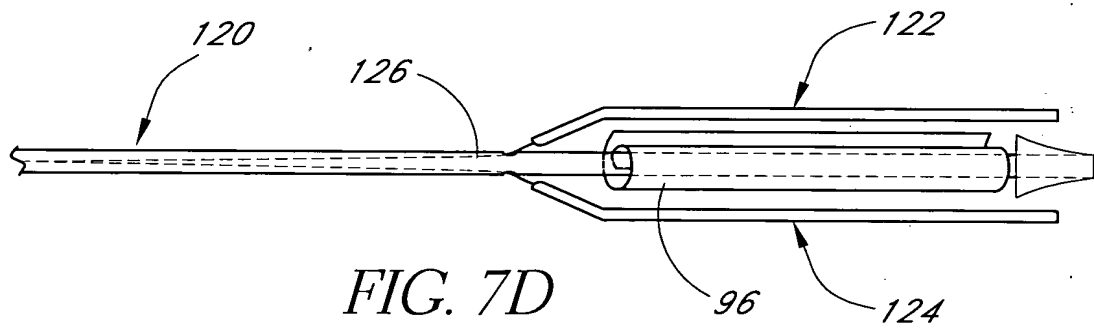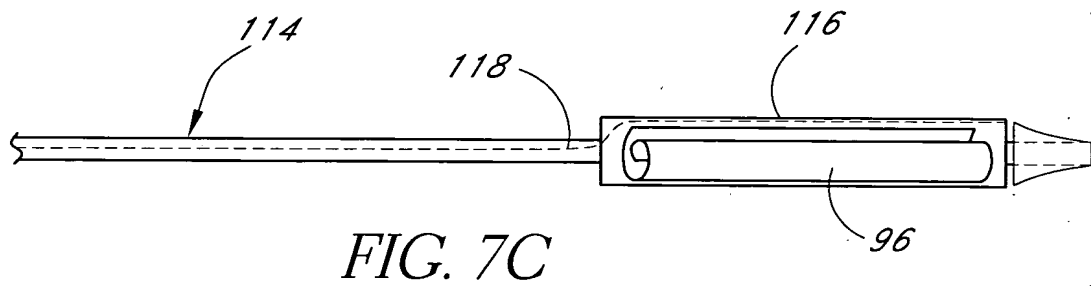

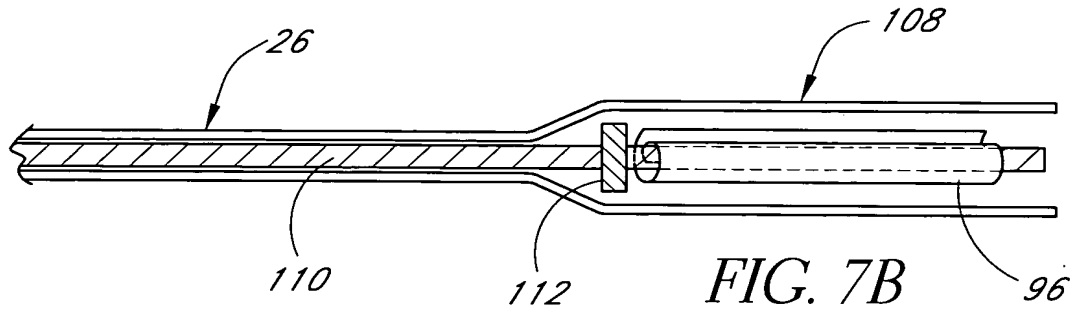

9/22

FIG. 7F

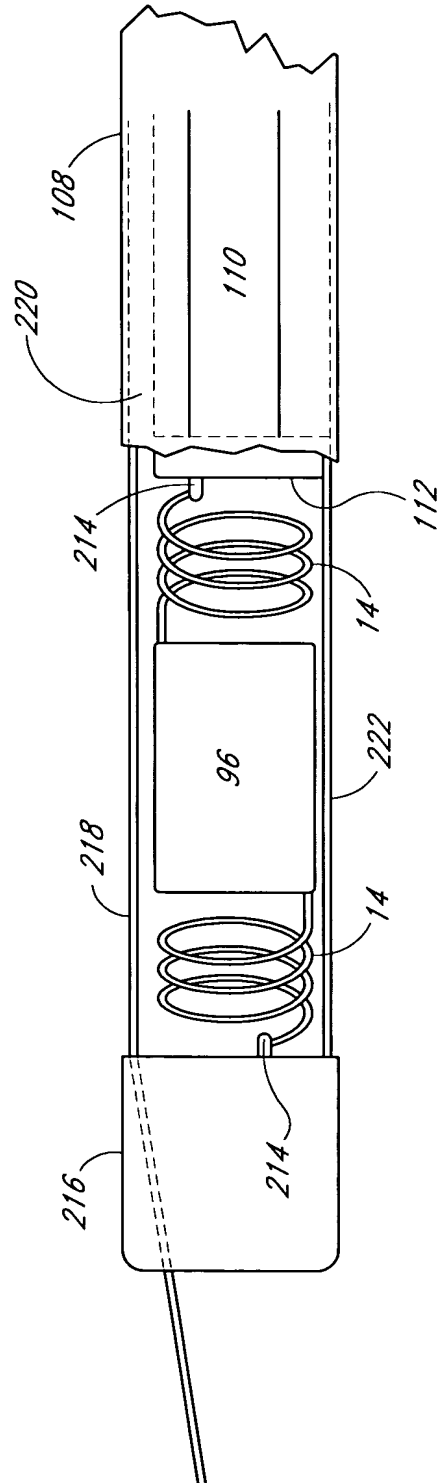

10/22

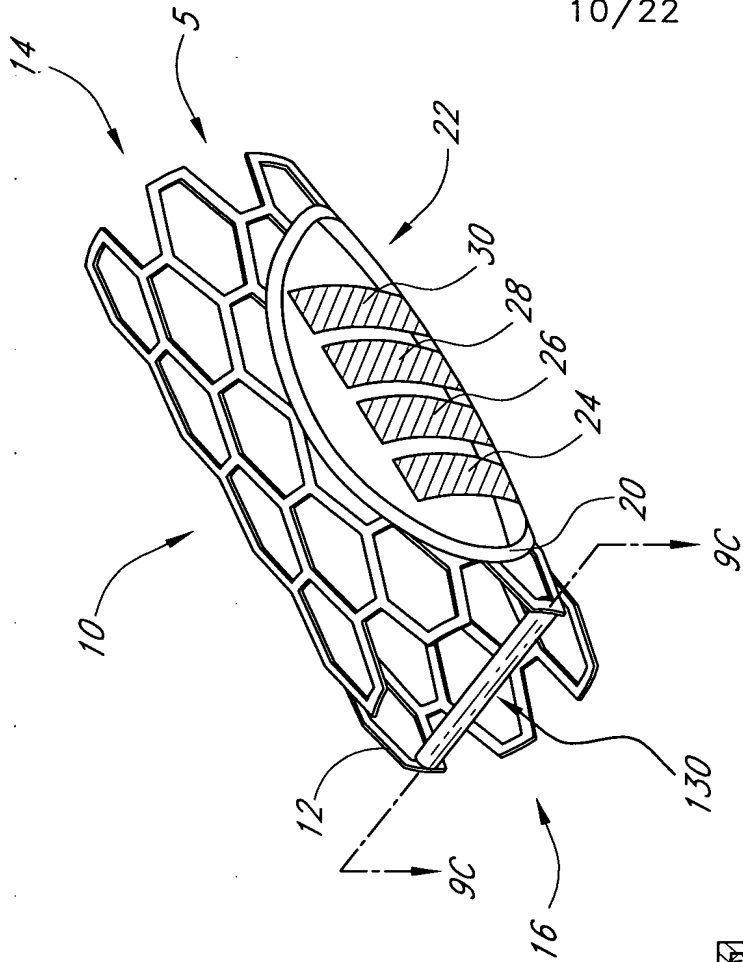


FIG. 9B

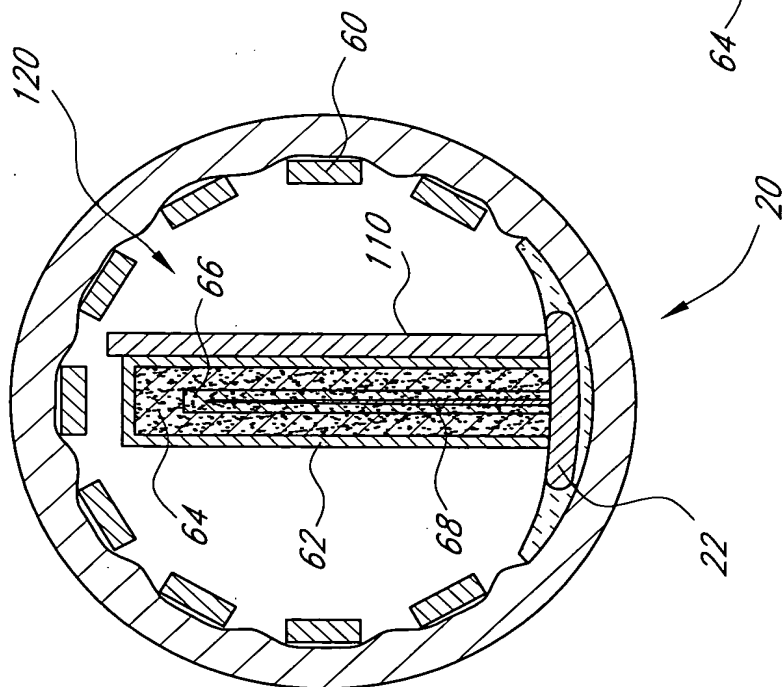


FIG. 9A

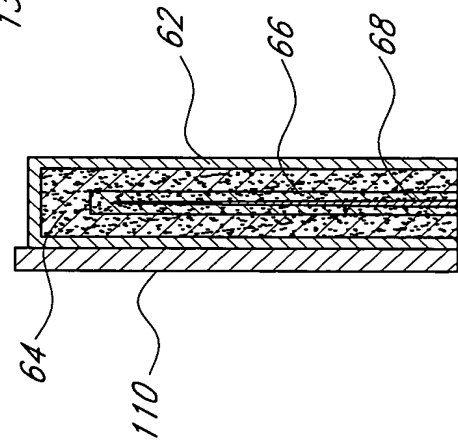


FIG. 9C

11/22

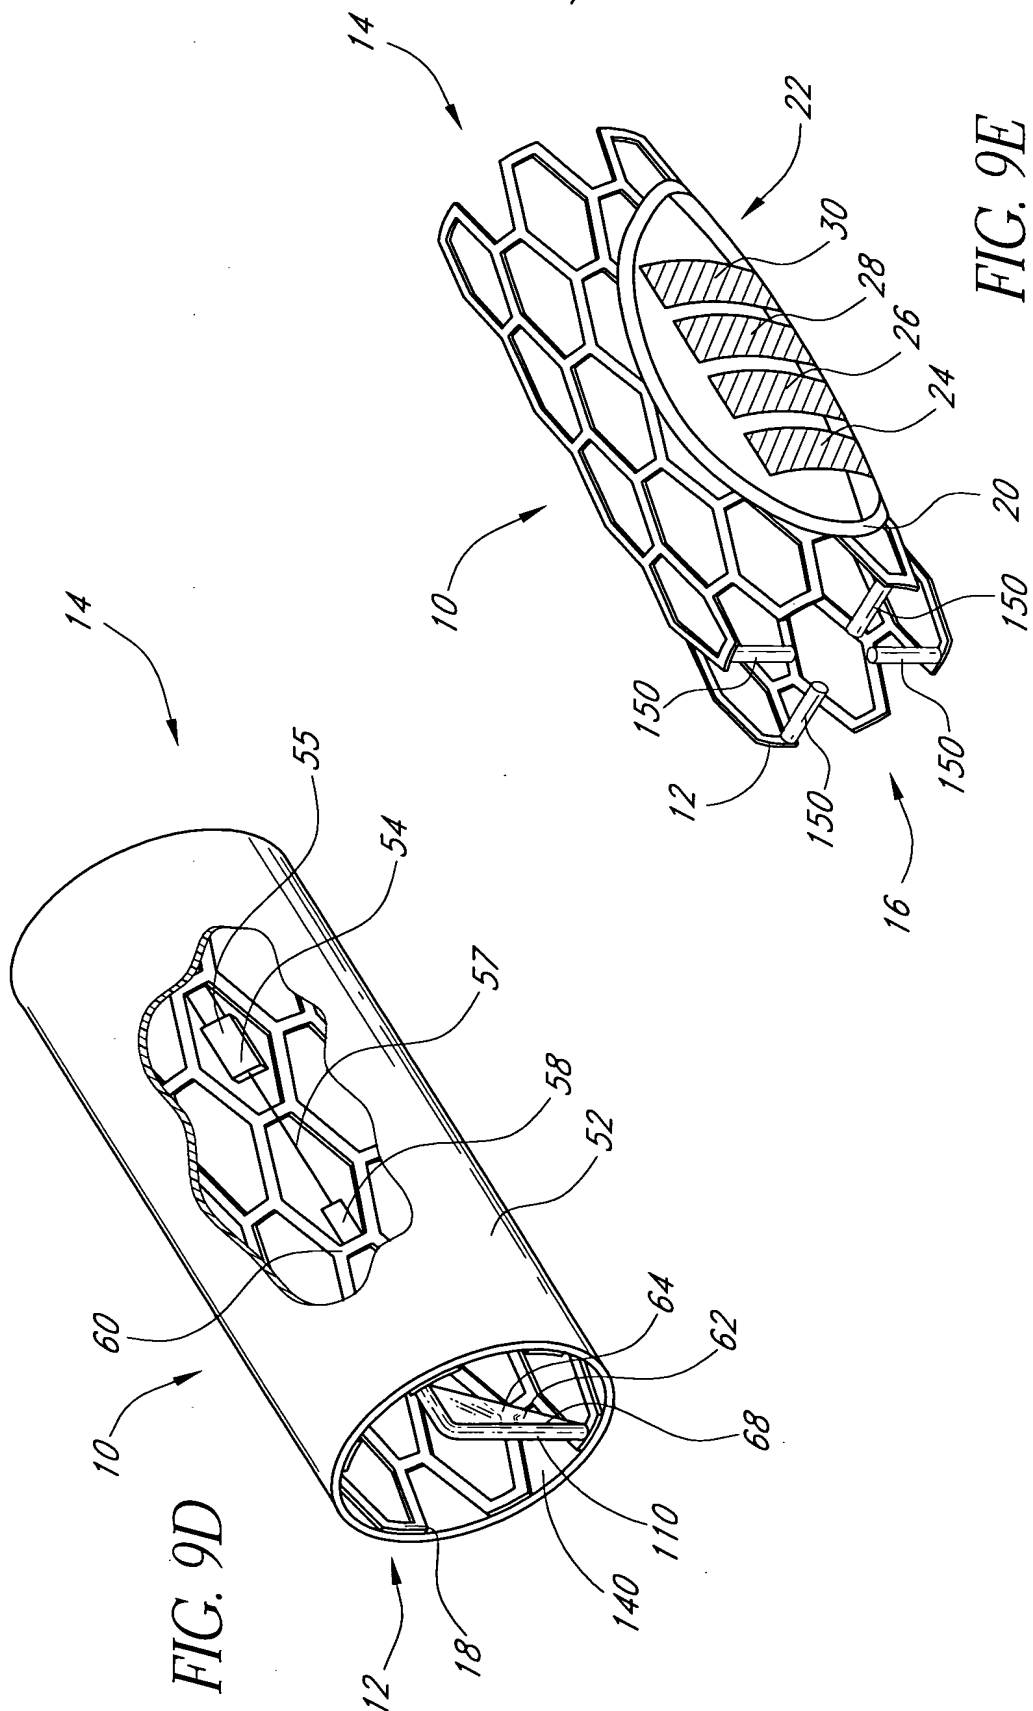


FIG. 9D

FIG. 9E

FIG. 10


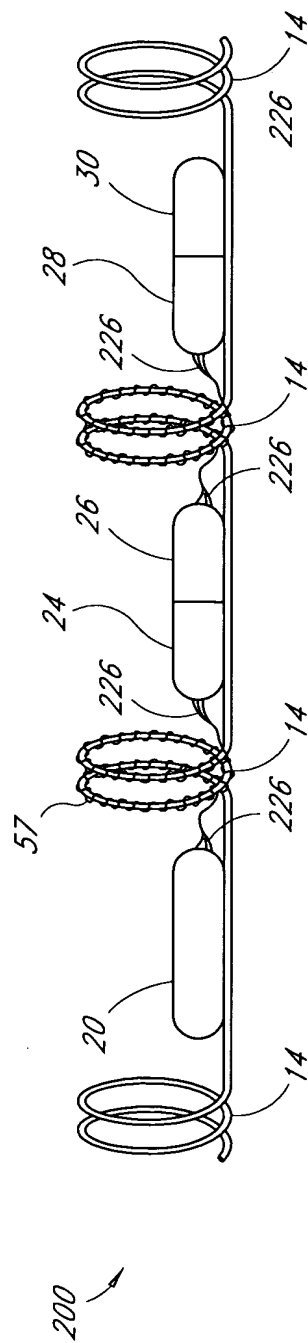


FIG. 11

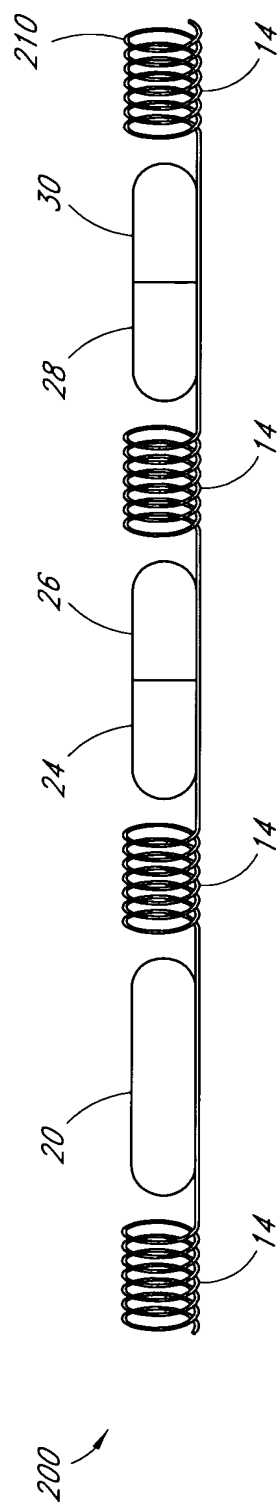

14/22

FIG. 12

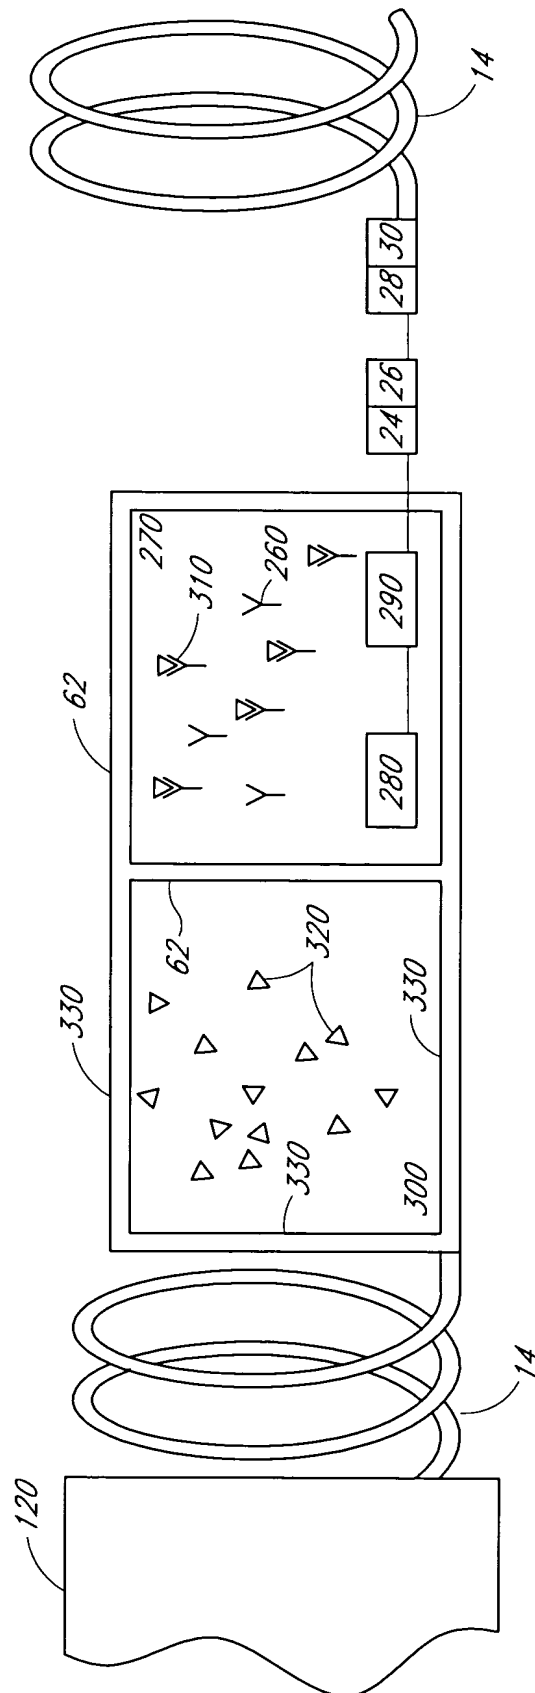


FIG. 14A

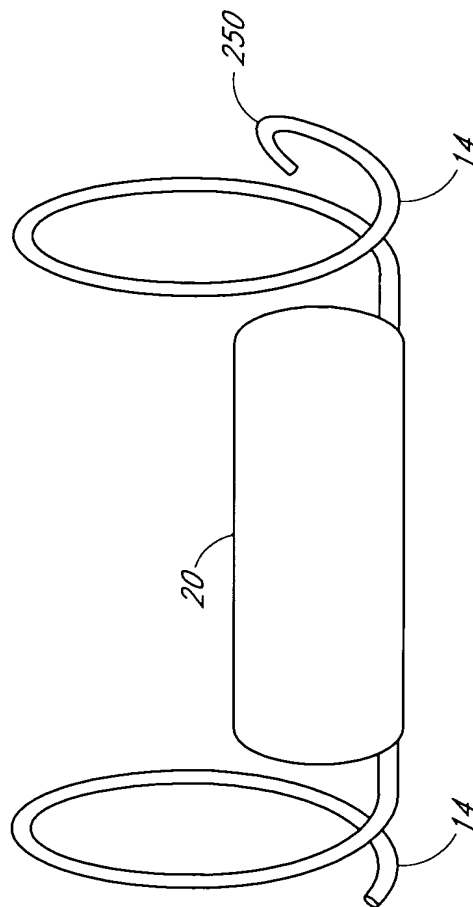
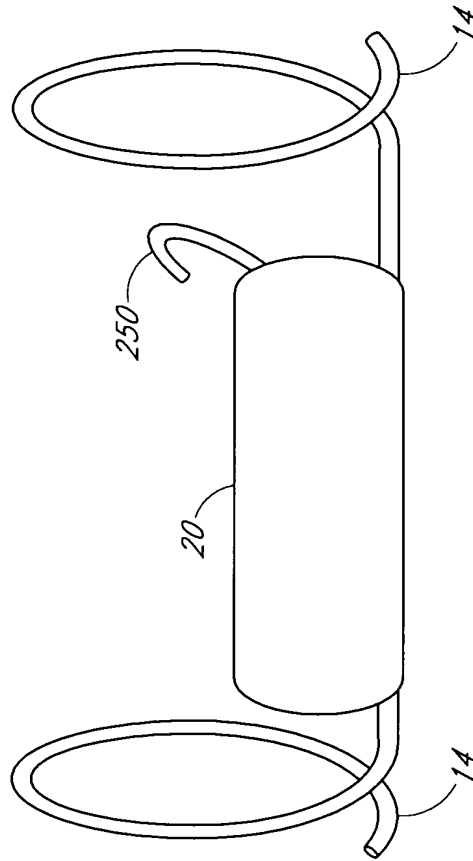


FIG. 14B



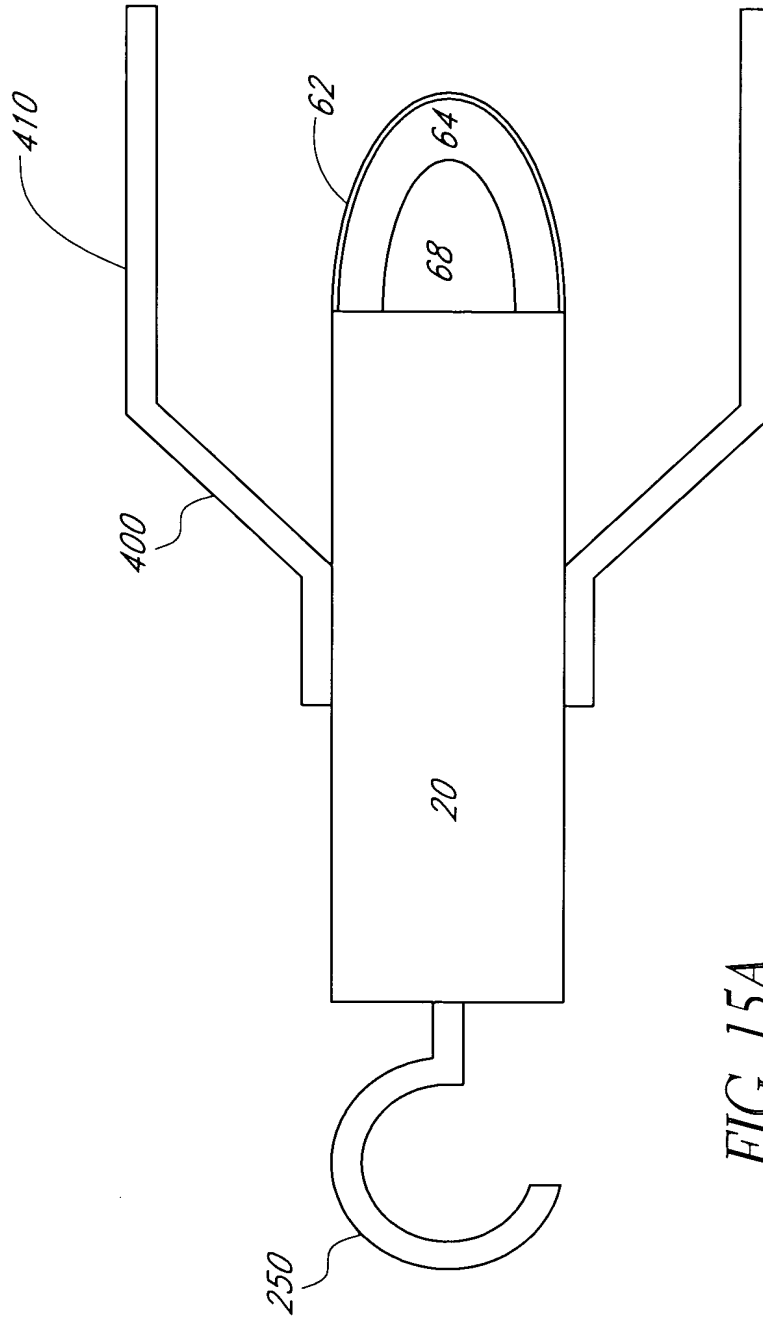


FIG. 15B



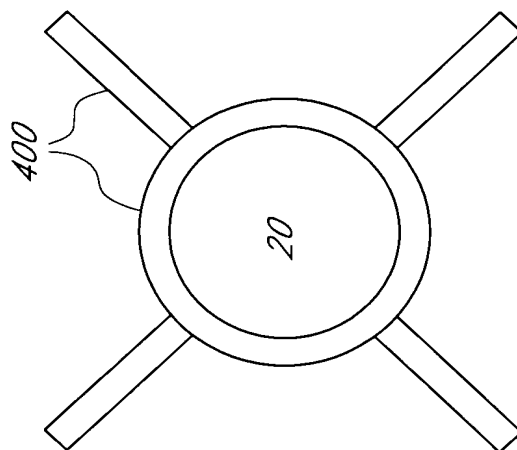


FIG. 16

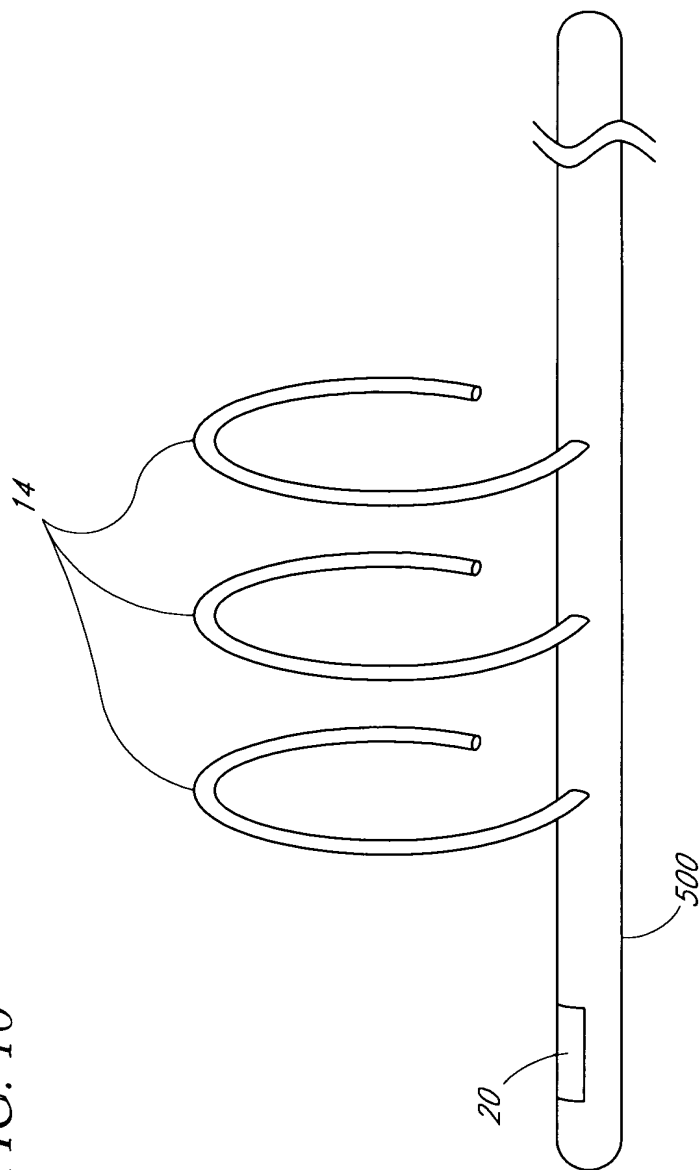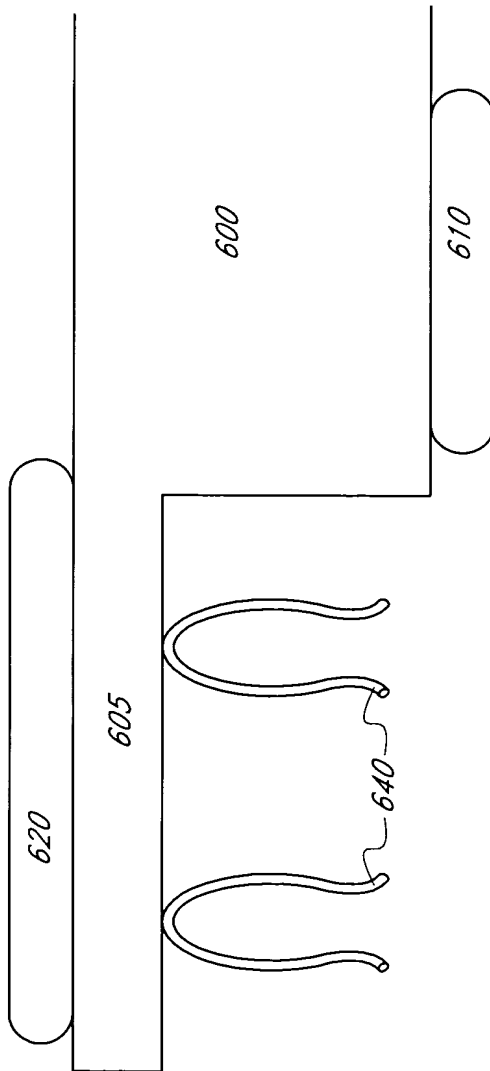

20/22

FIG. 17A



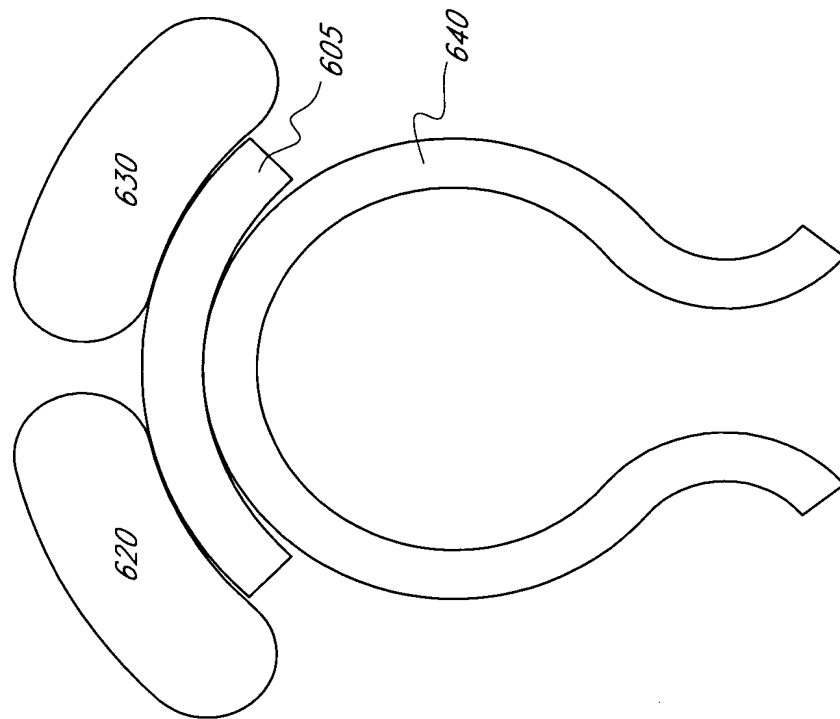


FIG. 17B

FIG. 18

